

openheart Impact of device landing zone calcification patterns on paravalvular regurgitation after transcatheter aortic valve replacement with different next-generation devices

Victor Mauri ,¹ Thomas Frohn,¹ Florian Deuschl,² Kawa Mohamed,³ Kathrin Kuhr,¹ Andreas Reimann,¹ Maria Isabel Körber,¹ Niklas Schofer,² Matti Adam,¹ Kai Friedrichs,³ Elmar W Kuhn,¹ Smita Scholtz,³ Volker Rudolph,³ Thorsten C W Wahlers,⁴ Stephan Baldus,⁵ Navid Mader,⁴ Ulrich Schäfer,² Tanja K Rudolph³

► Additional material is published online only. To view please visit the journal online (<http://dx.doi.org/10.1136/openhrt-2019-001164>).

To cite: Mauri V, Frohn T, Deuschl F, *et al.* Impact of device landing zone calcification patterns on paravalvular regurgitation after transcatheter aortic valve replacement with different next-generation devices. *Open Heart* 2020;**7**:e001164. doi:10.1136/openhrt-2019-001164

Received 30 August 2019
Revised 18 February 2020
Accepted 26 March 2020



© Author(s) (or their employer(s)) 2020. Re-use permitted under CC BY-NC. No commercial re-use. See rights and permissions. Published by BMJ.

For numbered affiliations see end of article.

Correspondence to
Professor Tanja K Rudolph;
trudolph@hdz-nrw.de

ABSTRACT

Objective Residual paravalvular regurgitation (PVR) has been associated to adverse outcomes after transcatheter aortic valve replacement (TAVR). This study sought to evaluate the impact of device landing zone (DLZ) calcification on residual PVR after TAVR with different next-generation transcatheter heart valves.

Methods 642 patients underwent TAVR with a SAPIEN 3 (S3; n=292), ACURATE *neo* (NEO; n=166), Evolut R (ER; n=132) or Lotus (n=52). Extent, location and asymmetry of DLZ calcification were assessed from contrast-enhanced CT imaging and correlated to PVR at discharge.

Results PVR was ≥moderate in 0.7% of S3 patients, 9.6% of NEO patients, 9.8% of ER patients and 0% of Lotus patients (p<0.001), and these differences remained after matching for total DLZ calcium volume. The amount of DLZ calcium was significantly related to the degree of PVR in patients treated with S3 (p=0.045), NEO (p=0.004) and ER (p<0.001), but not in Lotus patients (p=0.698). The incidence of PVR ≥moderate increased significantly over the tertiles of DLZ calcium volume (p=0.046). On multivariable analysis, calcification of the aortic valve cusps, LVOT calcification and the use of self-expanding transcatheter aortic valve implantation (TAVI) prostheses emerged as predictors of PVR.

Conclusions The susceptibility to PVR depending on the amount of calcium was mainly observed in self-expanding TAVI prostheses. Thus, DLZ calcification is an important factor to be considered in prosthesis selection for each individual patient, keeping in mind the trade-off between PVR reduction, risk of new pacemaker implantation and unfavourable valve haemodynamics.

INTRODUCTION

Over the last decade, transcatheter aortic valve replacement (TAVR) has evolved to the standard of care for the treatment of severe aortic stenosis in patients at intermediate

Key questions

What is already known about this subject?

- The extent of device landing zone (DLZ) calcification is an important risk factor for paravalvular regurgitation (PVR) after transcatheter aortic valve replacement (TAVR).

What does this study add?

- The relation between DLZ calcium and PVR differed between different TAVR devices with significantly higher susceptibility for DLZ calcium and, consequently, higher rates of PVR after TAVR with self-expanding devices compared with balloon or mechanically expanding devices. Besides PVR, also the need for new permanent pacemaker implantation and valve haemodynamics differed significantly between the devices.

How might this impact on clinical practice?

- Our data might help clinicians to consider the advantages and disadvantages of each prosthesis for an individualised prosthesis selection.

or high risk for conventional surgery and expansion to lower risk populations is on the rise.^{1–3} Paravalvular regurgitation (PVR) is a major limitation of TAVR, being linked to increased mortality.^{4,5} The rapid extension of interventional therapy has been facilitated by significant advancements in device technology resulting in lower rates of periprocedural complications.⁶ Device landing zone (DLZ) calcifications which impact sealing of the transcatheter heart valves (THVs) to the aortic valve cusps (AVCs) and left ventricular outflow tract (LVOT) have been identified as the main predictor of PVR in numerous

studies with first-generation devices.^{7–12} With the introduction of next-generation TAVR devices with dedicated sealing mechanisms, the rate of relevant PVR decreased significantly, however to a variable extent with different prostheses due to differences in device design, implantation mechanism and radial force. The aim of this study was to determine the impact of extent and distribution of DLZ calcium on PVR with several next-generation valves in order to facilitate prosthesis selection since comparative data on different device systems of the current generation are lacking.

METHODS

In total, 792 consecutive patients underwent TAVR for severe native aortic stenosis with various next-generation transcatheter valves at three centres. For CT analysis, 150 patients were excluded because of missing or low-quality CT (n=73) or transthoracic echocardiography (TTE) data (n=70), or conversion to conventional surgery (n=7). Six hundred forty-two patients with complete data were included into the study cohort. Prostheses used included the SAPIEN 3 (S3; Edwards Lifesciences, Irvine, CA, USA), ACURATE *neo* (NEO; Boston Scientific, Marlborough, MA, USA), Evolut R (ER; Medtronic, Minneapolis, MN, USA) and Lotus (Boston Scientific). Prosthesis selection was at the discretion of the operating physicians considering individual patient characteristics. The study was conducted in accordance with German and European regulations. Informed consent was waived by the ethics committee due to the retrospective nature of the analysis. Patients were considered not suitable for surgical aortic valve replacement by the local interdisciplinary heart-team. Pre-procedural routine work-up included echocardiography, coronary angiography and contrast-enhanced multi-slice computed tomography (MSCT). Valve sizing was based on the manufacturer's recommendations. Primary endpoint was the degree of PVR at discharge. Secondary clinical and safety VARC-2 endpoints are reported on the overall population in order to reduce an inherent bias for certain complications in case of presenting only patients with both CT and TTE data.

MSCT data analysis

All MSCT data analysis was performed by two independent observers who were unaware of outcome measures (interobserver variability for total calcium volume: 47.8 ± 123.6 mm³, intraclass correlation coefficient 0.98). Images were acquired on a dual source CT scanner (Siemens) with a slice thickness of 1 mm and 40 mL of intravenously administered Accupaque contrast agent. The aortic annulus was defined as a virtual basal plane at the nadirs of the valve cusps. The DLZ was defined as the composite of the AVC region (basal plane to the lower coronary ostium) and the LVOT (from basal plane 10 mm into the left ventricle). The calcium volume in the DLZ was measured by using an automated volume-scoring

tool (3mensio Medical Imaging) with an empiric starting threshold of 500 Hounsfield units (HU). The threshold was subsequently adjusted manually (steps of 20 HU) in each patient depending on the patient's individual density of luminal contrast medium for best discrimination between calcium and contrast medium. Both AVC and LVOT were subdivided into three regions of interest along the AVCs and analysed separately (online supplementary figure 1).

Area oversizing was calculated using the formula $\text{THV} = (\text{nominal area}/\text{annulus area} - 1) \times 100$, and perimeter oversizing accordingly. Eccentricity of the aortic annulus was evaluated with an index calculated as $1 - (\text{minimum diameter}/\text{maximum diameter})$. Asymmetry of calcium distribution was calculated as maximum absolute difference in calcium volume between leaflet sectors for both AVC and LVOT.

Evaluation of residual PVR

Residual PVR was analysed by two observers based on pre-discharge TTE using both quantitative and qualitative parameters according to the VARC-2 recommendations.

Statistics

Categorical variables are reported as frequencies and percentages, continuous variables as mean \pm SD or median (IQR), as applicable. Differences between THV groups were evaluated using Fisher's exact test for categorical variables and Kruskal-Wallis test for continuous variables. Kendall's τ correlation coefficients were calculated for the comparison of patients with different degrees of PVR. An ordinal logistic regression model was fitted to estimate the impact of AVC calcification, LVOT calcification and valve type (reference: S3) on the degree of PVR. Asymmetry was not considered in the model as asymmetry and calcification are highly correlated (Pearson's correlation coefficient $r=0.613$ for AVC calcium/asymmetry; $r=0.934$ for LVOT calcium/asymmetry). Case-matching was performed based on total DLZ calcium volume in a nearest neighbour fashion (4:3:2:1, 390 matched patients: S3: n=156; NEO: n=117; ER: n=78; Lotus: n=39) with an average SD tolerance of $6.6\% \pm 2.7\%$. Two-sided p values <0.05 were considered statistically significant. All analyses were performed using IBM SPSS Statistics V.22.

RESULTS

Patient population and DLZ characteristics

A total of 642 patients undergoing TAVR for severe aortic stenosis with a next-generation transcatheter device, including the SAPIEN 3 (n=292), ACURATE *neo* (n=166), Evolut R (n=132) or Lotus (n=52), were analysed. Baseline and DLZ characteristics were significantly different between the different treatment groups (table 1). In the overall cohort, mean age was 82.0 ± 5.8 years, 58.3% were female and patients had an intermediate to high risk for surgery (EuroSCORE I: $22.8\% \pm 15.9\%$; EuroSCORE II: $4.4\% \pm 4.0\%$). A transfemoral, transapical and transaortic

Table 1 Patient characteristics

	All n=642	SAPIEN 3 n=292	ACURATE neo n=166	Evolut R n=132	Lotus n=52	P value
Baseline and procedural characteristics						
Age (years)	82.0±5.8	81.2±6.4	82.9±4.8	83.1±5.5	81.4±5.7	0.01
Female sex	374 (58.3)	127 (43.5)	123 (74.1)	96 (92.7)	28 (53.8)	<0.001
BMI (kg/m ²)	27.3±8.1	27.6±10.1	27.6±5.7	25.9±5.9	28.5±6.4	0.007
BSA (m ²)	1.82±0.22	1.87±0.22	1.79±0.19	1.74±0.21	1.89±0.25	<0.001
Baseline creatinine (mg/dL)	1.27±0.78	1.34±0.82	1.19±0.57	1.19±0.81	1.40±1.00	0.007
EuroSCORE I (%)	22.8±15.9	24.3±17.2	22.1±15.0	21.5±13.6	19.8±15.7	0.122
EuroSCORE II (%)	4.6±4.1	4.8±4.4	4.3±4.1	4.3±3.3	4.7±4.6	0.791
Pre-existing pacemaker	73 (11.4)	36 (12.3)	16 (9.7)	14 (10.6)	7 (13.5)	0.795
Predilatation	359 (56.5)	128 (44.0)	151 (92.6)	33 (25.6)	47 (90.4)	<0.001
Postdilatation	82 (12.9)	12 (4.1)	41 (25.2)	28 (21.7)	1 (1.9)	<0.001
Comorbidities						
COPD	110 (17.1)	66 (22.6)	21 (12.7)	15 (11.4)	8 (15.4)	0.009
Peripheral artery disease	132 (20.6)	73 (25.0)	33 (19.9)	17 (12.9)	9 (17.3)	0.032
Diabetes	200 (31.2)	92 (31.5)	54 (32.5)	39 (29.5)	15 (28.8)	0.939
Hypertension	584 (91)	258 (88.4)	157 (94.6)	121 (91.7)	48 (92.3)	0.16
Coronary artery disease	402 (62.2)	174 (59.6)	111 (66.9)	83 (62.9)	34 (65.4)	0.464
Previous cardiac surgery	124 (19.3)	82 (28.1)	20 (12.0)	20 (15.2)	2 (3.8)	<0.001
Atrial fibrillation	262 (40.9)	123 (42.1)	63 (38.2)	57 (43.2)	19 (36.5)	0.717
Device landing zone characteristics						
Area (mm ²)	479.9±102.8	510.5±104.2	454.9±98.9	449.4±94.1	464.7±80.3	<0.001
Perimeter (mm)	79.1±8.1	81.6±8.3	77.1±7.8	76.8±7.2	77.5±6.6	<0.001
AVC calcium volume (mm ³)	616 (406–979)	697 (425–1059)	581 (359–834)	590 (375–879)	718 (414–1005)	0.009
NCC (mm ³)	273 (156–4449)	286 (168–481)	251 (150–378)	253 (149–384)	336 (177–514)	0.048
RCC (mm ³)	175 (96–305)	197 (114–333)	154 (87–244)	165 (87–305)	181 (86–337)	0.007
LCC (mm ³)	157 (89–276)	172 (99–323)	142 (73–261)	142 (88–251)	170 (88–251)	0.028
LVOT calcium volume (mm ³)	25 (4–114)	28 (4–109)	19 (2–98)	33 (5–140)	24 (2–158)	0.488
LVOT _{NC} (mm ³)	6 (0–38)	6 (0–36)	4 (0–31)	9 (0–44)	7 (0–49)	0.341
LVOT _{RC} (mm ³)	3 (0–8)	0 (0–8)	0 (0–8)	1 (0–8)	0 (0–6)	0.811
LVOT _{LC} (mm ³)	4 (0–33)	4 (0–34)	3 (0–16)	4 (0–48)	6 (0–71)	0.672
Total DLZ calcium volume (mm ³)	683 (441–1073)	740 (472–1175)	626 (388–882)	620 (411–983)	819 (434–12 289)	0.006
AVC absolute asymmetry (mm ³)	199±156	213±162	171±127	185±133	247±226	0.07
LVOT absolute asymmetry (mm ³)	56±92	52±82	51±93	71±115	63±80	0.456

Values are mean±SD, n (%) or median (IQR).

AVC, aortic valve cusp; BMI, body mass index; BSA, body surface area; COPD, chronic obstructive pulmonary disease; DLZ, device landing zone; LVOT, left ventricular outflow tract; NCC/RCC/LCC, non-/right/left coronary cusp.

approach was chosen in 93.9%, 5.0% and 1.1% of patients, respectively.


Total DLZ calcium volume was 834±569 mm³ with significant differences between the different THV with highest average calcium volume in the Lotus group and lowest calcium volumes in the NEO group (p=0.006). Median calcium volume of the aortic valve cusps was 616 (406–979) mm³, with the non-coronary cusp being the most calcified region, followed by the right and left coronary cusp. Median LVOT calcium volume was 25 (4–114) mm³, being individually widely dispersed. The mean AVC

maximum absolute asymmetry was 199±156 mm³, and LVOT absolute asymmetry was 56±92 mm³.

Residual PVR and clinical endpoints

The occurrence and degree of residual PVR differed significantly between the devices (figure 1A). PVR was ≥moderate in 0.7% of S3 patients, 9.6% of NEO patients, 9.8% of ER patients and 0.0% of Lotus patients, respectively (p<0.001). Due to significant differences in DLZ calcification between the different devices (being lower in self-expanding devices), patients were case-matched

A

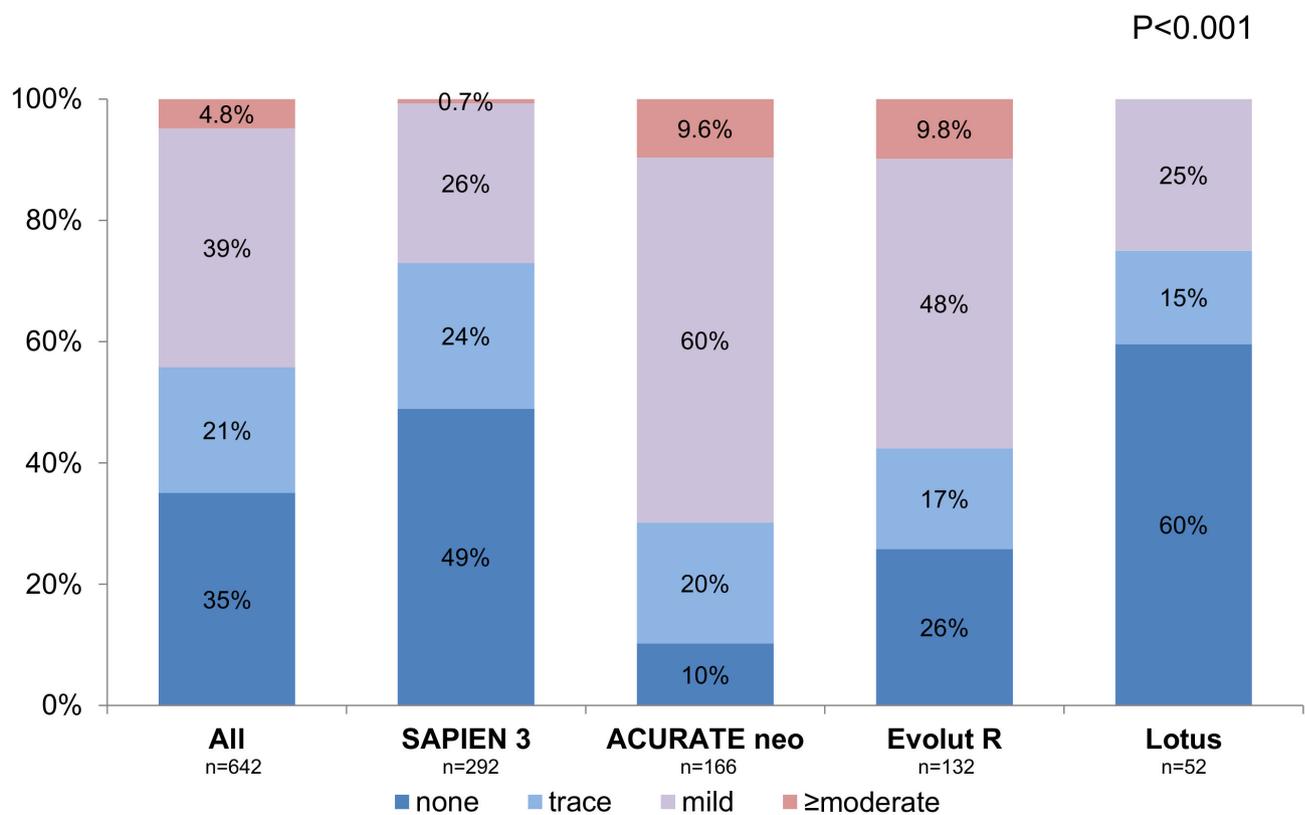

B

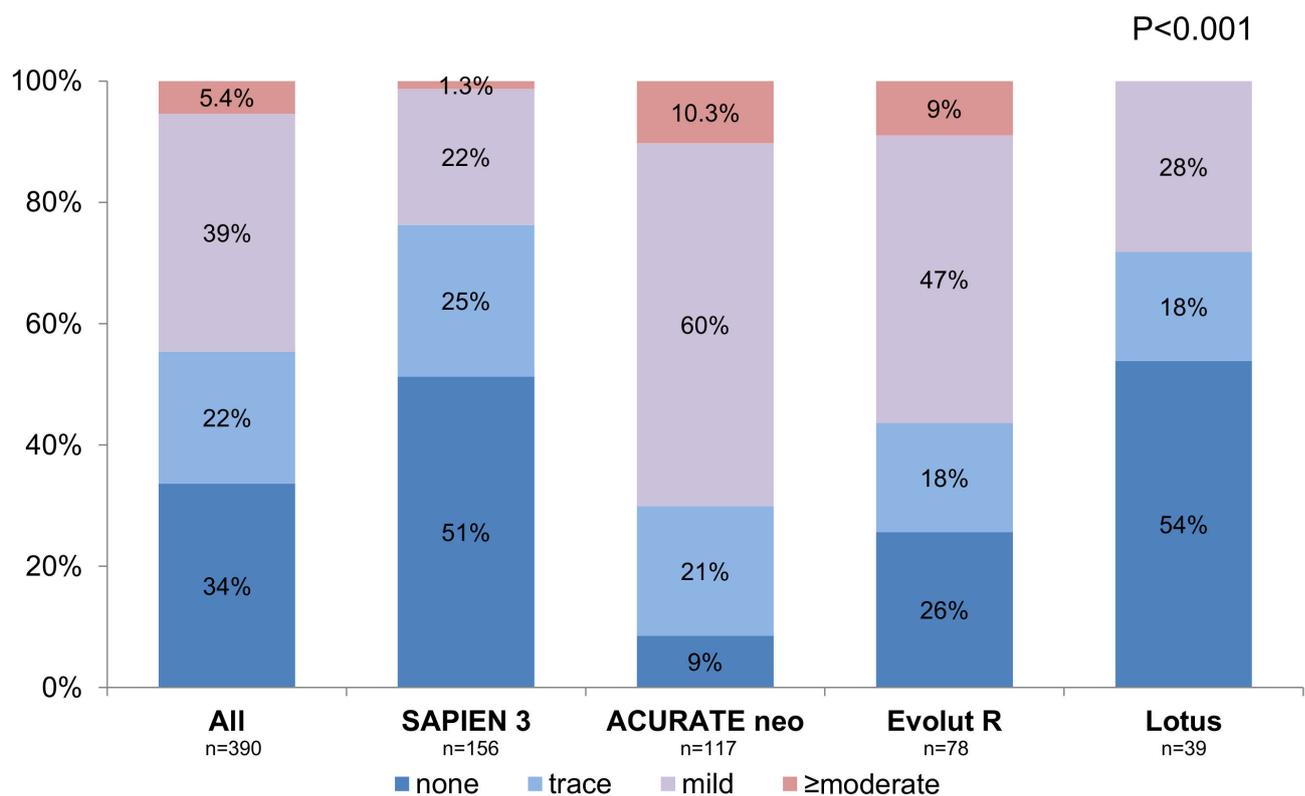


Figure 1 Degree of residual paravalvular regurgitation. (A) Degree of paravalvular regurgitation (PVR) with different devices. (B) Degree of PVR with different devices after matching for total device landing zone calcium volume.

according to total DLZ calcium. After matching, total DLZ calcium was well balanced between the different groups (866 ± 593 mm³; $p=0.999$). However, the degree

of residual PVR remained significantly different between groups, with PVR \geq moderate being present in 1.3% of

Table 2 Clinical endpoints

	SAPIEN 3	ACURATE neo	Evolut R	Lotus	P value
	n=382	n=189	n=157	n=63	
30-day mortality	15 (3.9)	3 (1.6)	7 (4.5)	5 (7.9)	0.105
Major vascular complication	15 (3.9)	2 (1.1)	4 (2.5)	5 (7.9)	0.042
Major/life-threatening bleeding	21 (5.5)	4 (2.1)	3 (1.9)	6 (9.5)	0.019
Stroke	8 (2.1)	3 (1.6)	5 (3.2)	3 (4.8)	0.397
Early safety	38 (9.9)	7 (3.7)	14 (8.9)	12 (19.0)	0.002
New permanent pacemaker*	36 (11.3)	18 (10.4)	31 (21.8)	20 (37.7)	<0.001
$\Delta P_{\text{mean post TAVI}}$ (mm Hg)	12.3±4.7	9.2±3.9	8.6±4.3	13.5±5.0	<0.001

Values are n (%) or mean±SD.

*Patients with pre-existing pacemaker were excluded from these calculations. TAVI, transcatheter aortic valve implantation.

S3, 10.3% of NEO, 9.0% of ER and 0% of Lotus patients ($p<0.001$; [figure 1B](#)).

Haemodynamics were significantly different between the studied devices with significantly lower mean transvalvular gradients after TAVR with the self-expanding NEO or ER compared with S3 and Lotus ([table 2](#)). Permanent pacemaker implantation (PPI) rates (excluding patients with pre-existing pacemaker) were 11.3%, 10.4%, 21.8% and 37.7% in S3, NEO, ER and Lotus patients,

respectively ($p<0.001$). Rates of 30-day mortality and stroke were numerically different without being statistically significant, whereas the unadjusted rates of major vascular complications and major or life-threatening bleeding were significantly different with highest event rates in the Lotus group ([table 2](#)).

DLZ calcification patterns and residual PVR

Higher DLZ calcium load was significantly related to the occurrence and degree of PVR in patients treated with the self-expanding NEO ($p=0.004$) and ER ($p<0.001$), but to a lesser extent after S3 implantation ($p=0.045$) and not related in Lotus valve patients ($p=0.698$ [figure 2A–D](#)).

In the overall cohort, the rate of PVR \geq moderate increased significantly over the 3 tertiles of total DLZ calcium volume (2.3%, 4.7% and 7.5%, respectively). However, this increase was predominantly observed in NEO and ER patients, but not in S3 and Lotus patients ($p=0.046$; [figure 3](#)). Combined ROC-curve analysis was performed for NEO and ER patients to predict PVR \geq moderate (AUC 0.70; $p<0.001$). The risk of PVR \geq moderate was significantly higher above a DLZ calcium load of 1257.9 mm^3 (8.6 vs 33.3%; OR 5.3, 95% CI 2.4 to 11.6; $p<0.001$).

Besides the susceptibility for PVR depending on total DLZ calcium volume, also the influence of calcium location and distribution as assessed by absolute sector asymmetry varied between the different devices. In NEO and ER patients, both AVC and LVOT calcium were predictive


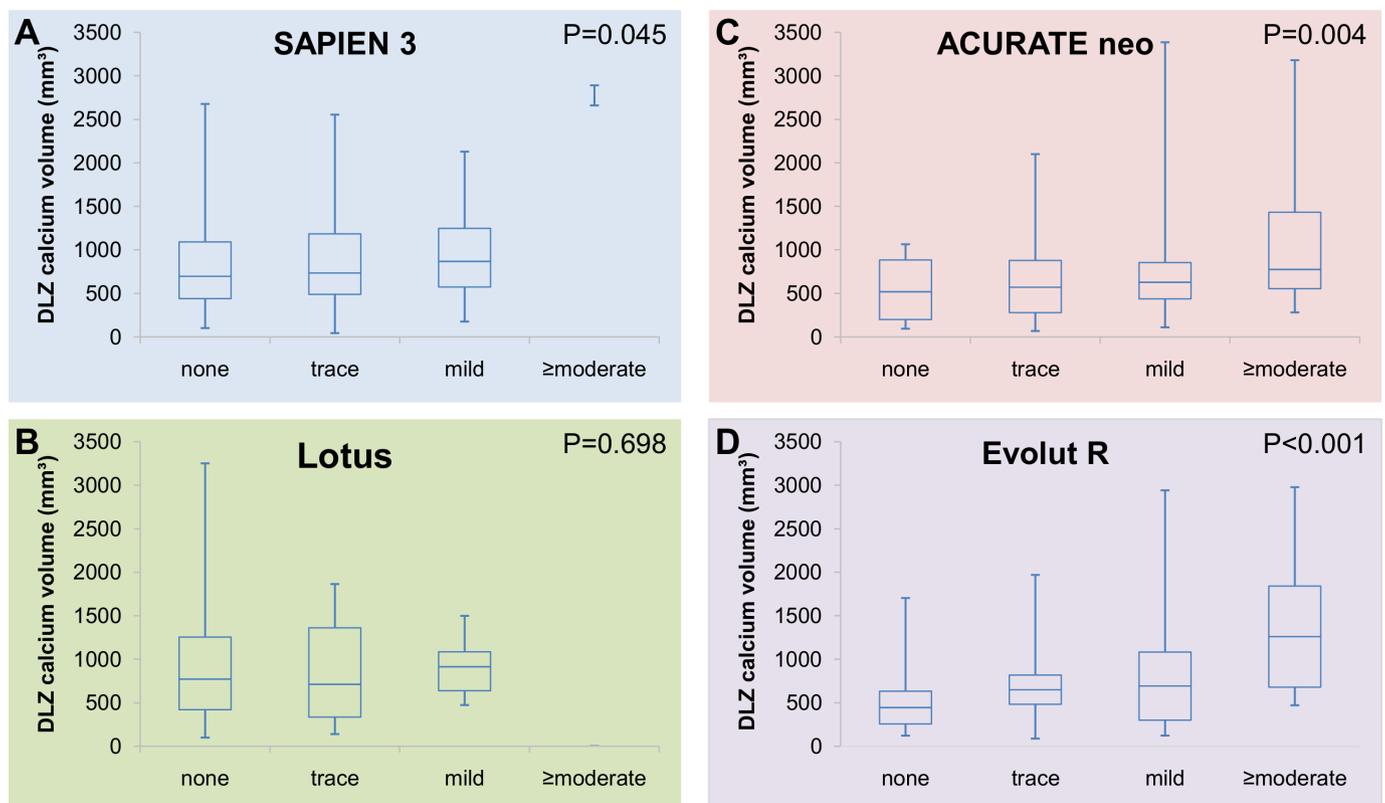


Figure 2 Device landing zone (DLZ) calcium volume and paravalvular regurgitation (PVR) with different devices. Relation between DLZ calcification and degree of PVR in patients treated with (A) SAPIEN 3; (B) Lotus; (C) ACURATE neo; (D) Evolut R.

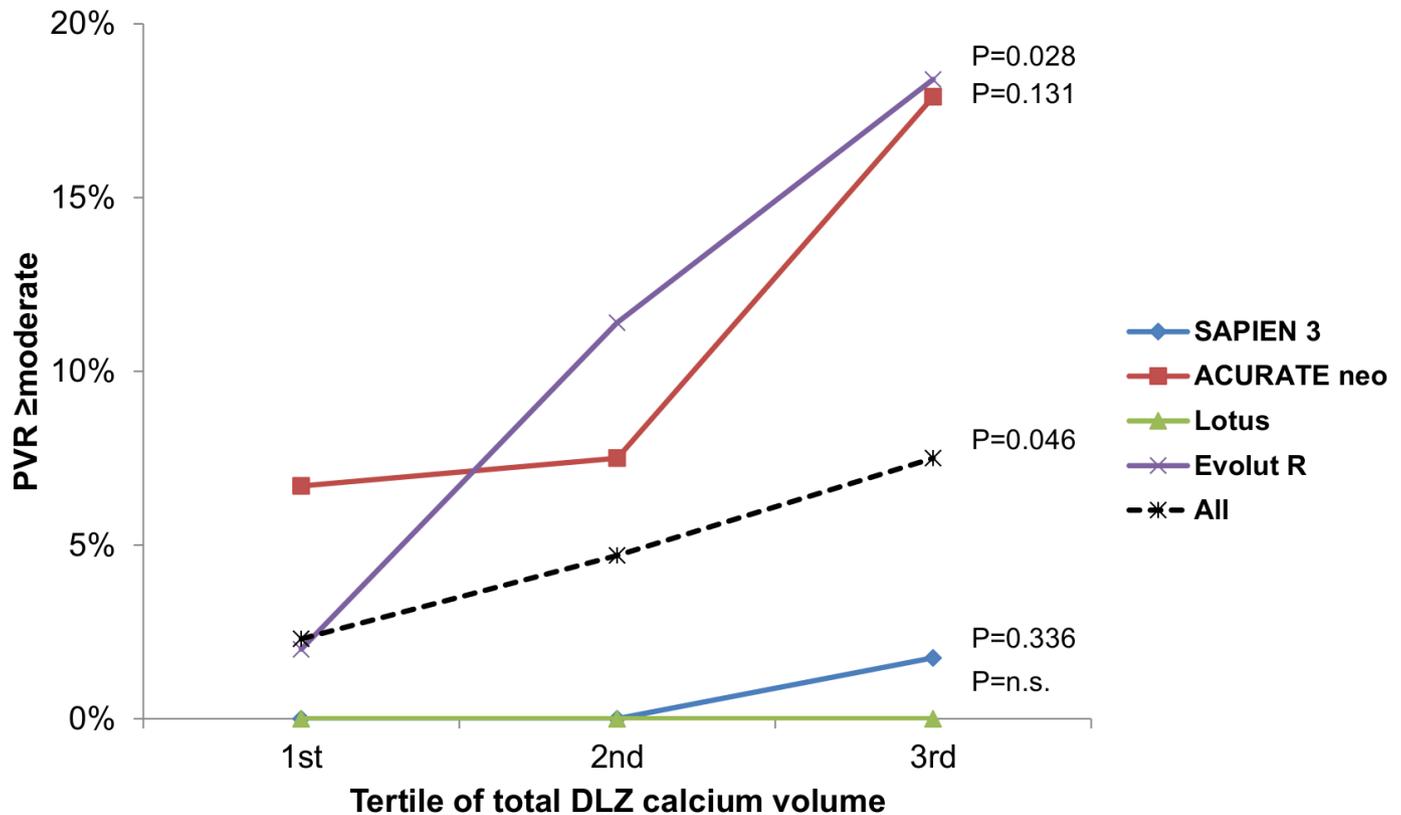

Patient numbers according to group and tertile			
	1st	2nd	3rd
SAPIEN 3	30	31	39
ACURATE <i>neo</i>	36	40	23
Evolut R	38	33	29
Lotus	33	23	44

Figure 3 Paravalvular regurgitation (PVR) \geq moderate according to total calcium volume. The rate of patients with PVR \geq moderate increased significantly over the 3 tertiles of device landing zone (DLZ) calcium volume, and this increase was driven by increasing rates of PVR \geq moderate after self-expanding transcatheter aortic valve replacement.

for the degree of PVR, whereas only AVC calcium load predicted PVR in S3 patients, but not LVOT calcification. Both AVC and LVOT asymmetry were related to the degree of PVR in NEO patients, but only LVOT asymmetry in ER patients. In patients treated with S3 and Lotus, asymmetry was not related to the degree of PVR. Annular eccentricity or prosthesis sizing in relation to the native annulus was not associated to the degree of PVR in any of the devices. The details of the different calcification patterns in relation to the degree of PVR are given in online supplementary table 1.

An ordinal logistic regression model to predict the degree of PVR was fitted including valve type, AVC and LVOT calcification. Thereby, the use of NEO or ER (with the SAPIEN 3 as reference), AVC calcium and LVOT calcium emerged as independent predictors of PVR, whereas the use of Lotus did not (table 3).

DISCUSSION

To our best knowledge, we present the currently broadest study addressing the impact of device landing zone calcification patterns on PVR after TAVR with a variety of different next-generation prostheses. The main findings

Table 3 Ordinal logistic regression analysis for the prediction of PVR

	OR	95% CI	P value
Valve type (SAPIEN 3 reference)			
ACURATE <i>neo</i>	7.2	5.0 to 10.5	<0.001
Evolut R	3.8	2.5 to 5.7	<0.001
Lotus	0.7	0.4 to 1.3	0.212
AVC calcium	1.005	1.002 to 1.009	0.004
LVOT calcium	1.014	1.003 to 1.026	0.013

ORs for calcium per 10 mm³ increase.

AVC, aortic valve cusp; LVOT, left ventricular outflow tract; PVR, paravalvular regurgitation.

of our study are (1) higher DLZ calcium volume and asymmetry as well as the use of a self-expanding device result in higher degrees of PVR; (2) the relation between DLZ calcium and PVR differed between the tested devices with significantly higher susceptibility for DLZ calcium and consequently, higher rates of PVR \geq moderate after TAVR with self-expanding devices; (3) despite PVR, also the need for new permanent pacemaker implantation, valve haemodynamics and short-term clinical outcome differed between the devices which may be taken into consideration in an individualised prosthesis selection.

Numerous studies have shown the negative impact of PVR \geq moderate on mortality after TAVR, some suggesting even mild PVR might have a negative impact on outcome.^{4 5} Several risk factors for PVR have been identified for first-generation valves, including DLZ calcification, valve type, undersizing and annulus eccentricity.^{5 7–12} Our study showed a significantly higher susceptibility to DLZ calcium of the self-expanding NEO and ER compared with the balloon-expandable S3 and the mechanically expandable Lotus resulting in significantly higher rates of PVR after self-expanding TAVR. The observed PVR rates of all valves are within the range of previously published studies.^{13–17} Notably, the degree of PVR seems unrelated to DLZ calcification patterns in Lotus treated patients, although the low patient number in this treatment group precludes any further conclusion. The difference in patients with PVR \geq moderate was most pronounced in the tertile of patients with highest DLZ calcium load, putting these patients at a highly increased risk for relevant PVR (figure 3). Conversely, the rate of PVR was acceptably low with all studied devices in the lower third of patients. Based on these data, any device might be used in patients with mild to moderate calcifications, whereas in patients with higher calcium load, a balloon-expandable or mechanically expandable THV might be advantageous to avoid PVR. This has to be counterweighed with the rare risk of aortic root or LVOT injury that has previously been associated with LVOT calcification in smaller studies.¹⁸ In our cohort, we did not see an association of LVOT calcification and aortic root complications (n=3). However, the incidence of aortic root injury decreased over the last years, most likely due to spreading of CT-based sizing strategies and growing operator experience.¹⁹ This may also be the reason that—in contrast to previous studies²⁰—we did not see an association of undersizing or annulus eccentricity and PVR in our study.

Beyond the total extent of DLZ calcium, also the location and asymmetry of calcification affected the studied devices to a variable degree. Again, the self-expanding devices were more susceptible to PVR in asymmetrically calcified anatomies, whereas there was no influence of an asymmetric calcium distribution after balloon-expandable or mechanically expandable TAVR.

In line with previously published data, transvalvular gradients were most favourable after TAVR with the self-expanding devices and significantly higher after

balloon-expandable and even more pronounced after mechanically expandable devices.²¹ Elevated transvalvular gradients and consecutively calculated parameters such as prosthesis–patient mismatch are well-known predictors of mortality, recurrence of heart failure symptoms, rehospitalisation and structural valve deterioration after surgical aortic valve replacement and TAVR.^{22–25}

Besides PVR, the unadjusted rates of other important endpoints which may affect long-term outcomes were different. Namely, in line with other contemporary studies, the rate of new-onset conduction disturbance requiring PPI were 10.4% and 11.3% for NEO and S3 treated patients, but significantly higher after TAVR with ER or Lotus (21.8% and 37.7%), respectively.^{26–28} However, it has to be noted that in contrast to PVR, the reported secondary endpoints are more prone to be influenced by differences in baseline patient characteristics and should consequently be interpreted with caution.

Lower risk populations with longer inherent life expectancy and higher levels of activity may be more prone to the negative effects of long-term right ventricular pacing or unfavourable haemodynamics compared with the initially treated high-risk patients. The current rapid expansion of TAVR indications to such lower risk populations¹ emphasises the need for a tailored prosthesis selection in each individual patient. Clinicians need to keep in mind the risk factors for certain complications, such as DLZ calcification patterns for PVR, as shown in this study, pre-existing conduction disturbances for new PPI, namely a pre-existing right bundle branch block, and for example, small annular dimensions for unfavourable haemodynamics. With current next-generation devices, there seems to be a trade-off between protection against PVR on one side, and the risk for new PPI or unfavourable haemodynamics on the other side that has to be considered in each individual patient and counterweighed along with the advantages and disadvantages of each valve system in order to achieve the best possible long-term results for our patients. None of the current studied devices seem to address all these issues in a favourable manner. Whether these limitations may be overcome by the further developed upcoming generation of TAVR devices, such as the S3 Ultra, the NEO AS, the Lotus Edge or the Evolut Pro, remains to be elucidated.

Study limitations

This study is a retrospective observational analysis with all inherent limitations. The individual valve choice in each patient was not randomised, but based on the best clinical knowledge of the operating heart-team at the time of procedure. Differences in DLZ calcium volume in the unadjusted dataset underline that the clinical decision on TAVR device was already based on the assumption that self-expanding TAVI prostheses are more susceptible to PVR. Thus, a certain confirmation bias cannot be fully excluded despite case-matching on DLZ calcium volume. Moreover, the reference standard for calcium quantification is the calculation of Agatston units using

non-contrast-enhanced CT scans. In the present study, calcium was measured using a CT protocol based on routinely acquired contrast-enhanced CT images since a contrast-free sequence is not performed routinely at many centres to avoid increased radiation exposure. The used method of calcium quantification has been previously shown to correlate well with the reference standard ($R=0.84$, $p<0.001$) and to be superior to methods with unadjusted thresholds, although calcium may be underestimated in patients with high aortic attenuation.²⁹ Finally, not all studied devices were commercially available during the complete study period. The Evolut Pro device which seems to be less susceptible to calcifications was not available during the study period and has therefore not been evaluated.

CONCLUSION

DLZ calcification predicted the degree of PVR after TAVR. The probability of PVR depending on the amount of calcium differed significantly with higher susceptibility in the self-expanding NEO and ER compared with the S3 or the Lotus. However, also permanent pacemaker implantation rates and transvalvular gradients differed significantly between the implanted devices. Thus, DLZ calcification is an important factor to be considered in prosthesis selection for each individual patient, keeping in mind the trade-off between PVR reduction, the occurrence of new-onset conduction disturbances requiring permanent pacemaker implantation and unfavourable valve haemodynamics.

Author affiliations

¹Heart Center, University of Cologne, Köln, Germany

²Department of Cardiology, University Hospital Hamburg Eppendorf University Heart Centre, Hamburg, Hamburg, Germany

³General und Interventional Cardiology/Angiology, Heart and Diabetes Center North Rhine-Westphalia, Bad Oeynhausen, Nordrhein-Westfalen, Germany

⁴Department of Cardiothoracic Surgery, Klinikum der Universität zu Köln, Klinik und Poliklinik für Herz- und Thoraxchirurgie, Cologne, Germany

⁵Department of Internal Medicine III, University of Cologne, Cologne, Germany

Acknowledgements We thank Anne Adams, M. Sc., from the Institute of Medical Statistics and Computational Biology, University of Cologne, for additional statistical advice.

Contributors VM and TR designed the study. TF, FD, KM, AR, NS, MA and SS performed CT analysis. VM, FD, KM, MIK, KF and NS performed TTE analysis. VM, TF, FD, KM, AR, MIK, NS, MA, KF, EWK and SS contributed to clinical patient data acquisition. VM and KK performed the statistical analyses. VM, VR and TR interpreted the data. VM and TR wrote the main manuscript text. EWK, VR, TCWW, SB, NM and US contributed to important intellectual content and critically revised the manuscript. TR supervised the work. All authors read and approved the final manuscript. We acknowledge support by the DFG Open Access Publication Funds of the Ruhr-Universität Bochum.

Funding The authors have not declared a specific grant for this research from any funding agency in the public, commercial or not-for-profit sectors.

Competing interests FD received speakers honoraria from Boston Scientific. NS received travel compensation from Edwards and speakers honoraria and travel compensation from Boston Scientific. VR received speakers honoraria from Medtronic. TCWW and NM are proctors for Edwards. SB is a proctor for Edwards and received a research grant from Edwards. US is proctor for Edwards and

Symetis SA and received research grants from Symetis SA and Edwards. TR is proctor for Boston Scientific and received speakers honoraria from Edwards, Medtronic and Boston Scientific/Symetis.

Patient consent for publication Not required.

Ethics approval The study was approved by the Ethics Committee of the University Hospital of Cologne (ID 19-1032).

Provenance and peer review Not commissioned; externally peer reviewed.

Data availability statement Data are available from the first author on reasonable request.

Open access This is an open access article distributed in accordance with the Creative Commons Attribution Non Commercial (CC BY-NC 4.0) license, which permits others to distribute, remix, adapt, build upon this work non-commercially, and license their derivative works on different terms, provided the original work is properly cited, appropriate credit is given, any changes made indicated, and the use is non-commercial. See: <http://creativecommons.org/licenses/by-nc/4.0/>.

ORCID iD

Victor Mauri <http://orcid.org/0000-0003-2678-3501>

REFERENCES

- 1 Popma JJ, Deeb GM, Yakubov SJ, *et al*. Transcatheter aortic-valve replacement with a self-expanding valve in low-risk patients. *N Engl J Med* 2019;380:1706–15.
- 2 Nishimura RA, Otto CM, Bonow RO, *et al*. 2014 AHA/ACC guideline for the management of patients with valvular heart disease: executive summary: a report of the American College of Cardiology/American Heart Association Task Force on Practice Guidelines. *Circulation* 2014;129:e650:2440–92.
- 3 Baumgartner H, Falk V, Bax JJ, *et al*. 2017 ESC/EACTS guidelines for the management of valvular heart disease. *Eur Heart J* 2017;38:616–64.
- 4 Kodali S, Pibarot P, Douglas PS, *et al*. Paravalvular regurgitation after transcatheter aortic valve replacement with the Edwards sapien valve in the PARTNER trial: characterizing patients and impact on outcomes. *Eur Heart J* 2015;36:449–56.
- 5 Athappan G, Patvardhan E, Tuzcu EM, *et al*. Incidence, predictors, and outcomes of aortic regurgitation after transcatheter aortic valve replacement: meta-analysis and systematic review of literature. *J Am Coll Cardiol* 2013;61:1585–95.
- 6 Athappan G, Gajulapalli RD, Tuzcu ME, *et al*. A systematic review on the safety of second-generation transcatheter aortic valves. *EuroIntervention* 2016;11:1034–43.
- 7 Seiffert M, Fujita B, Avanesov M, *et al*. Device landing zone calcification and its impact on residual regurgitation after transcatheter aortic valve implantation with different devices. *Eur Heart J Cardiovasc Imaging* 2016;17:576–84.
- 8 Buellesfeld L, Stortecky S, Heg D, *et al*. Extent and distribution of calcification of both the aortic annulus and the left ventricular outflow tract predict aortic regurgitation after transcatheter aortic valve replacement. *EuroIntervention* 2014;10:732–8.
- 9 Khaliq OK, Hahn RT, Gada H, *et al*. Quantity and location of aortic valve complex calcification predicts severity and location of paravalvular regurgitation and frequency of post-dilatation after balloon-expandable transcatheter aortic valve replacement. *JACC Cardiovasc Interv* 2014;7:885–94.
- 10 Ewe SH, Ng ACT, Schuijff JD, *et al*. Location and severity of aortic valve calcium and implications for aortic regurgitation after transcatheter aortic valve implantation. *Am J Cardiol* 2011;108:1470–7.
- 11 Feuchtnner G, Plank F, Bartel T, *et al*. Prediction of paravalvular regurgitation after transcatheter aortic valve implantation by computed tomography: value of aortic valve and annular calcification. *Ann Thorac Surg* 2013;96:1574–80.
- 12 Fonseca P, Figueiredo B, Almeida C, *et al*. Aortic valve calcium volume predicts paravalvular regurgitation and the need for balloon post-dilatation after transcatheter aortic valve implantation. *J Interv Cardiol* 2016;29:117–23.
- 13 Asch FM, Vannan MA, Singh S, *et al*. Hemodynamic and echocardiographic comparison of the Lotus and CoreValve transcatheter aortic valves in patients with high and extreme surgical risk: an analysis from the Reprise III randomized controlled trial. *Circulation* 2018;137:2557–67.
- 14 Noble S, Stortecky S, Heg D, *et al*. Comparison of procedural and clinical outcomes with Evolut R versus Medtronic CoreValve: a Swiss TAVI registry analysis. *EuroIntervention* 2017;12:e2170–6.

- 15 Enríquez-Rodríguez E, Amat-Santos IJ, Jiménez-Quevedo P, *et al.* Comparison of the hemodynamic performance of the balloon-expandable SAPIEN 3 versus self-expandable Evolut R transcatheter valve: a case-matched study. *Rev Esp Cardiol* 2018;71:735–42.
- 16 Pibarot P, Hahn RT, Weissman NJ, *et al.* Association of paravalvular regurgitation with 1-year outcomes after transcatheter aortic valve replacement with the SAPIEN 3 valve. *JAMA Cardiol* 2017;2:1208.
- 17 Lanz J, Kim W-K, Walther T, *et al.* Safety and efficacy of a self-expanding versus a balloon-expandable bioprosthesis for transcatheter aortic valve replacement in patients with symptomatic severe aortic stenosis: a randomised non-inferiority trial. *Lancet* 2019;394:1619–28.
- 18 Barbanti M, Yang T-H, Rodès Cabau J, *et al.* Anatomical and procedural features associated with aortic root rupture during balloon-expandable transcatheter aortic valve replacement. *Circulation* 2013;128:244–53.
- 19 Eggebrecht H, Vaquerizo B, Moris C, *et al.* Incidence and outcomes of emergent cardiac surgery during transfemoral transcatheter aortic valve implantation (TAVI): insights from the European Registry on Emergent Cardiac Surgery during TAVI (EuRECS-TAVI). *Eur Heart J* 2018;39:676–84.
- 20 Popma JJ, Reardon MJ, Khabbaz K, *et al.* Early clinical outcomes after transcatheter aortic valve replacement using a novel self-expanding bioprosthesis in patients with severe aortic stenosis who are suboptimal for surgery: results of the Evolut R U.S. Study. *JACC Cardiovasc Interv* 2017;10:268–75.
- 21 Mauri V, Kim WK, Abumayyaleh M, *et al.* Short-term outcome and hemodynamic performance of next-generation self-expanding versus balloon-expandable transcatheter aortic valves in patients with small aortic annulus: a multicenter propensity-matched comparison. *Circ Cardiovasc Interv* 2017;10.
- 22 Dayan V, Vignolo G, Soca G, *et al.* Predictors and outcomes of prosthesis-patient mismatch after aortic valve replacement. *JACC Cardiovasc Imaging* 2016;9:924–33.
- 23 Pibarot P, Dumesnil JG, Lemieux M, *et al.* Impact of prosthesis-patient mismatch on hemodynamic and symptomatic status, morbidity and mortality after aortic valve replacement with a bioprosthetic heart valve. *J Heart Valve Dis* 1998;7:211–8.
- 24 Rodriguez-Gabella T, Voisine P, Puri R, *et al.* Aortic bioprosthetic valve durability: incidence, mechanisms, predictors, and management of surgical and transcatheter valve degeneration. *J Am Coll Cardiol* 2017;70:1013–28.
- 25 Herrmann HC, Daneshvar SA, Fonarow GC, *et al.* Prosthesis-patient mismatch in patients undergoing transcatheter aortic valve replacement. *J Am Coll Cardiol* 2018;72:2701–11.
- 26 Möllmann H, Hengstenberg C, Hilker M, *et al.* Real-world experience using the ACURATE neo prosthesis: 30-day outcomes of 1,000 patients enrolled in the SAVI TF registry. *EuroIntervention* 2018;13:e1764–70.
- 27 Rampat R, Khawaja MZ, Hilling-Smith R, *et al.* Conduction abnormalities and permanent pacemaker implantation after transcatheter aortic valve replacement using the repositionable LOTUS device: the United Kingdom experience. *JACC Cardiovasc Interv* 2017;10:1247–53.
- 28 Reardon MJ, Van Mieghem NM, Popma JJ, *et al.* Surgical or transcatheter aortic-valve replacement in intermediate-risk patients. *N Engl J Med* 2017;376:1321–31.
- 29 Kim W-K, Renker M, Rolf A, *et al.* Accuracy of device landing zone calcium volume measurement with contrast-enhanced multidetector computed tomography. *Int J Cardiol* 2018;263:171–6.